



Final XRF/ICP Correlation

- ◆ 5% of Total= 90 Samples, focused near action level
 - 23% <400ppm, 43% 400-600 ppm, 34% >600 ppm

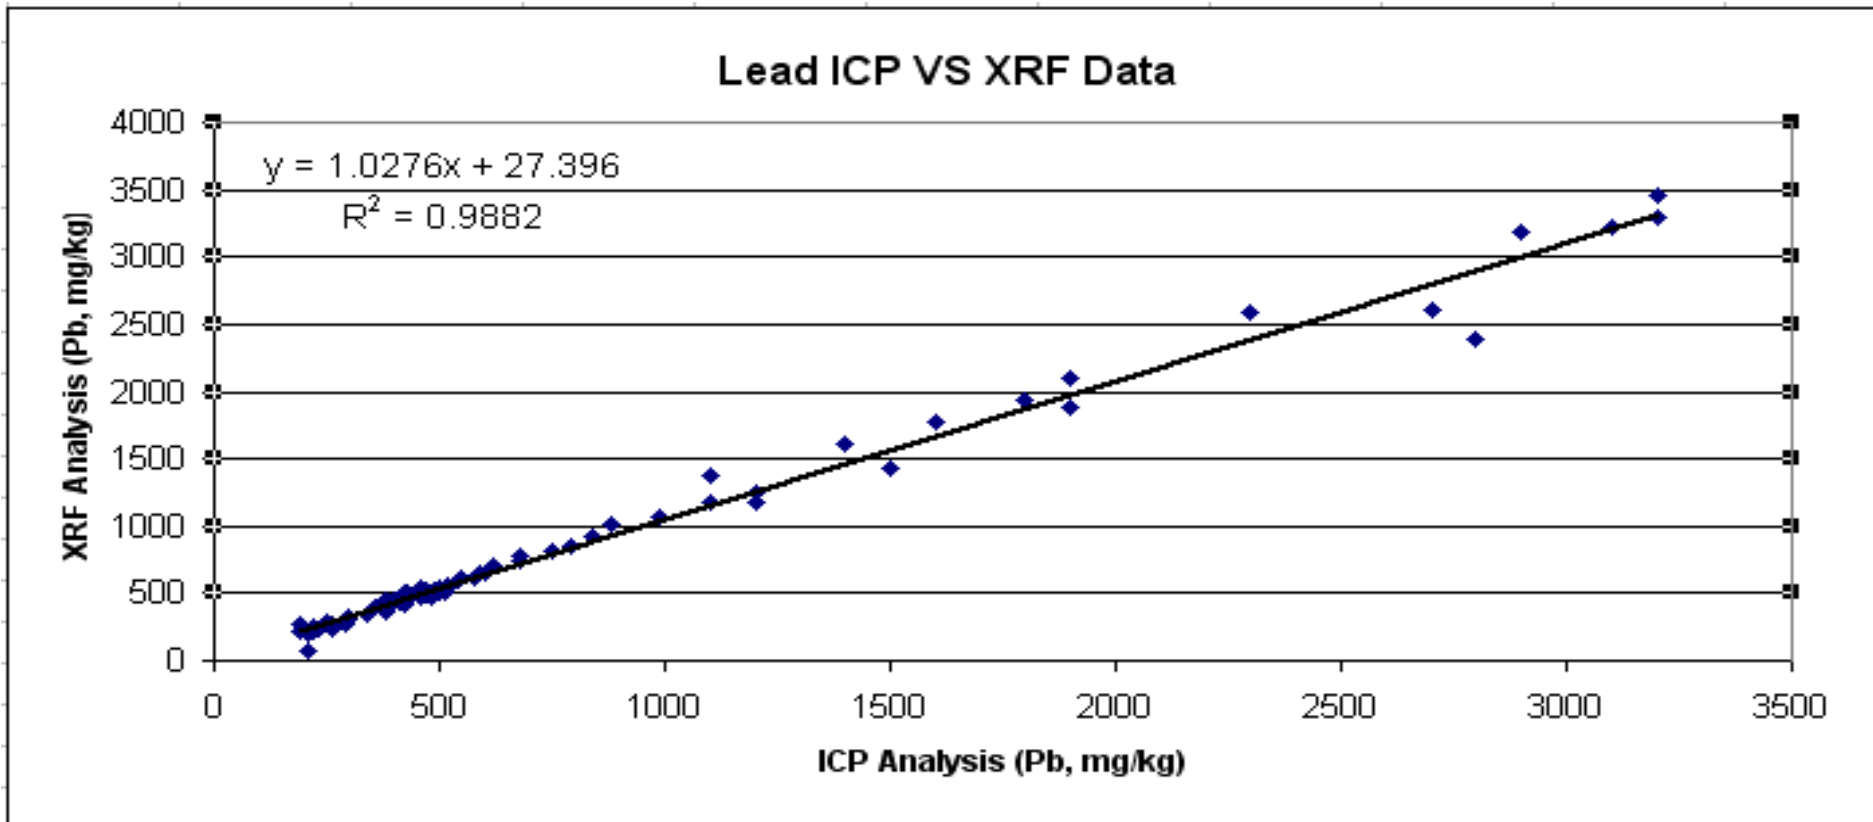

Cntrl Chart #	XRF Run #	Reading (ppm)	Date
1	24	532	10-14-09
2	25	549	10-14-09
3	47	504	10-14-09
4	8	525	10-15-09
5	24	541	10-15-09
6	64	556	10-15-09
7	81	519	10-15-09
8	116	484	10-15-09
9	5	541	10-19-09
10	10	518	10-19-09
11	38	529	10-19-09
12	67	520	10-19-09
13	5	535	10-20-09
14	26	507	10-20-09
15	43	540	10-20-09
16	54	500	10-20-09
17	5	510	10-21-09
18	26	532	10-21-09
19	44	543	10-21-09
20	80	525	10-21-09
21	2	447	10-22-09
22	40	541	10-22-09
23	69	516	10-22-09
24	82	518	10-22-09
25	2	506	10-23-09
26	39	547	10-23-09
27	64	537	10-23-09
28	77	528	10-23-09
29	5	472	10-26-09
30	47	534	10-26-09
31	62	517	10-26-09
32	5	486	10-27-09
33	28	532	10-27-09
34	2	512	10-28-09
35	35	502	10-28-09
36	2	572	10-29-09
37	40	525	10-29-09
38	52	485	10-29-09
39	78	504	10-29-09
40	101	487	10-29-09
41	2	535	10-30-09
42	24	551	10-30-09
43	43	514	10-30-09
44			

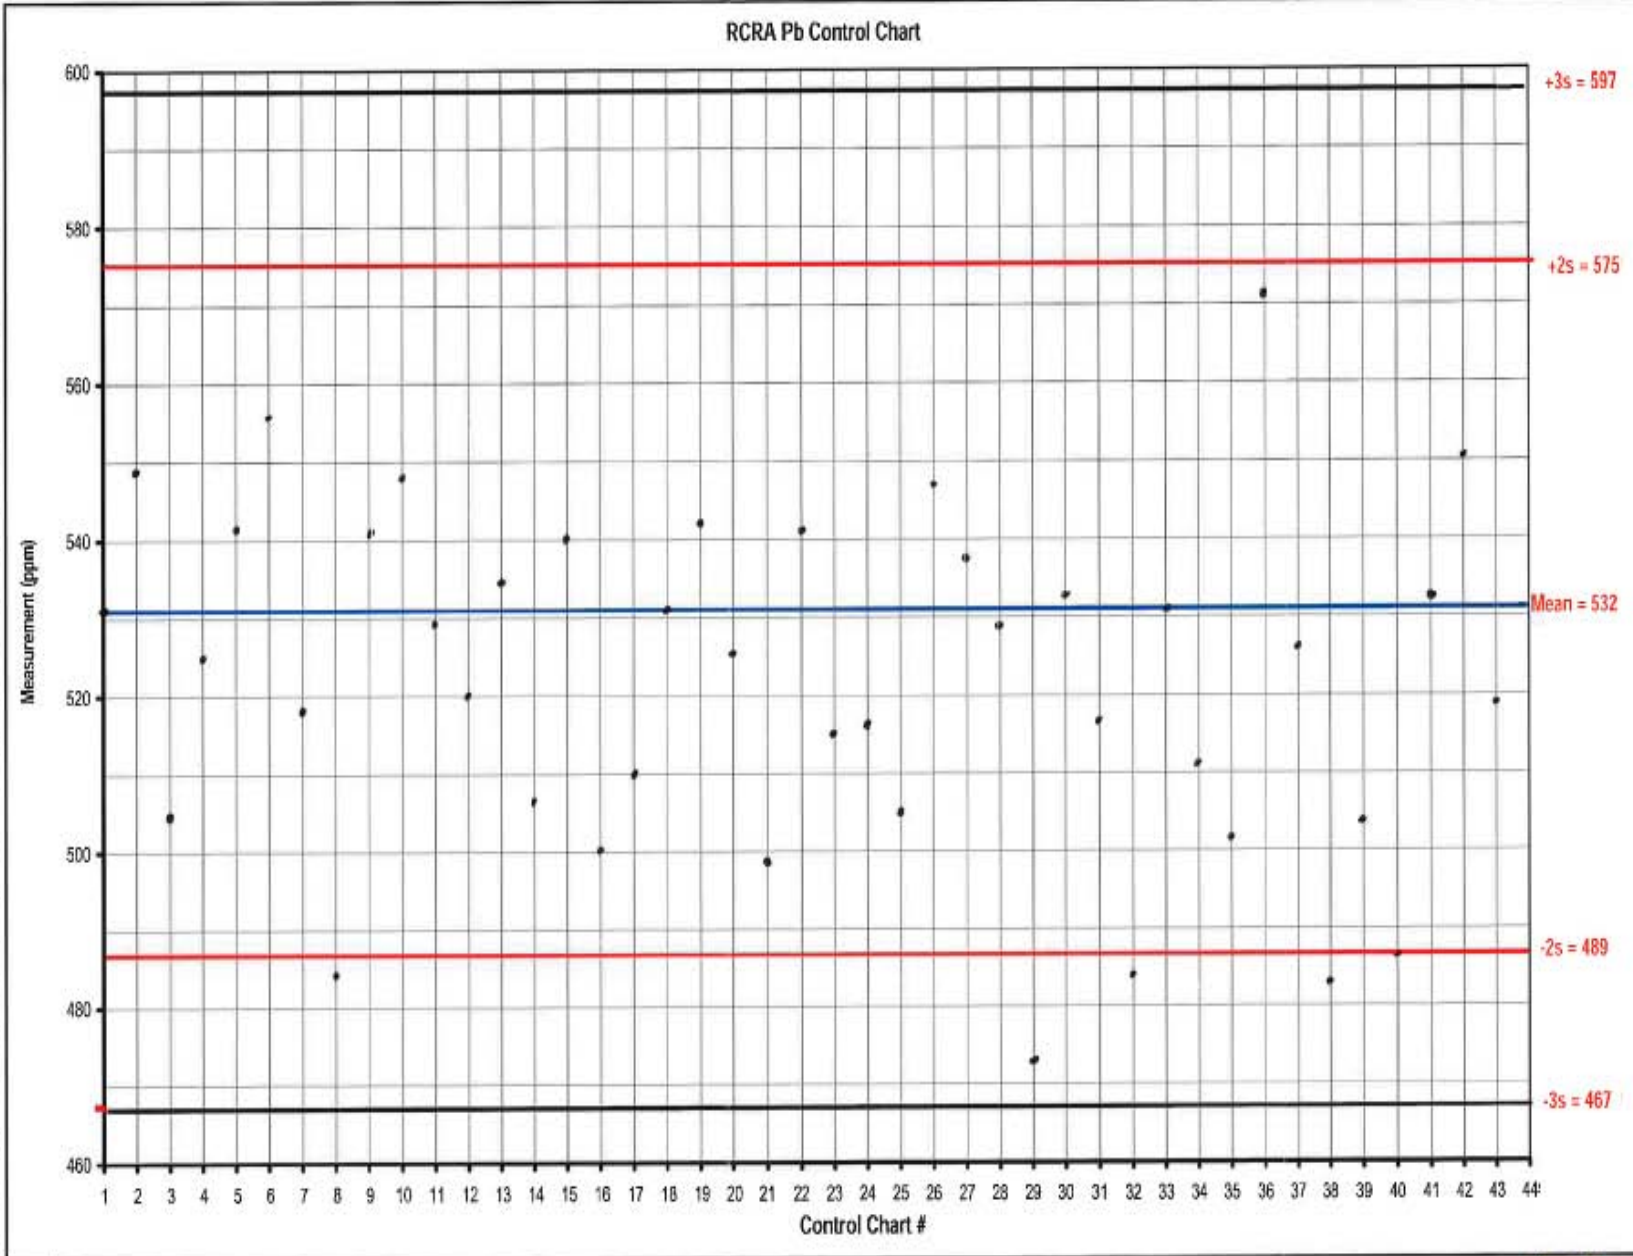

Personnel: Quinn Walker
 Signature: [Signature]

XRF Unit: Innov-X Alpha Series, Serial # 5740, Model # A-200AS, Rental # R7741

